

Certificate of Analysis


Date:	2025-07-18 12:27:21 -04:00	Moisture:	0.0%
Serial:	LL030645	Col Tests	20
LightLab	BW-LABS	Remaining:	
Operator:	DAIANA	CoA Revision:	1
Sample ID:		Calibration Exp:	2026-03-21
Method:	LightLab HPLC	Product:	Ultra Blend Infused Gummies
Test Type:	Gummy- Advanced Hemp Derived		Blue Raspberry
Weight / Volume:	4.5 g	SKU:	
Solvent:	40 ml	Batch:	MU0075
Temperature:	26.2 °C		
Cultivar:			
Notes:			

Cannabinoid Profile

Analyte	Per 4.500 g Serving (mg)	Per 1.0 Pieces(mg)	%	LOQ
Δ9-THC	1.1	1.1	0.024	0.041
CBD-A	ND	ND	ND	0.041
CBG-A	ND	ND	ND	0.041
CBD/CBG	ND	ND	ND	0.014
CBN	ND	ND	ND	0.041
CBC	ND	ND	ND	0.041
Δ8-THC*	41.8	41.8	0.93	0.041
Δ10-THC	ND	ND	ND	0.041
THCV	ND	ND	ND	0.041
Δ9-THC-O	ND	ND	ND	0.027
Δ8-THC-O	ND	ND	ND	0.041
HHC	10.2	10.2	0.23	0.027
Δ9-THCP	1.1	1.1	0.024	0.027
Terpenes			Low	
Total THC	ND	ND	ND	
Total Cannabinoids	54.2	54.2	1.2	

ND = Not Detected; n/a = Not Analyzed; LOQ = Limit of Quantification; Total THC = (0.877 x THC-A) + Δ9-THC; Total CBD = (0.877 x CBD-A) + CBD. * Δ8THC has lower precision and higher detection limit than other cannabinoids.

Chromatogram

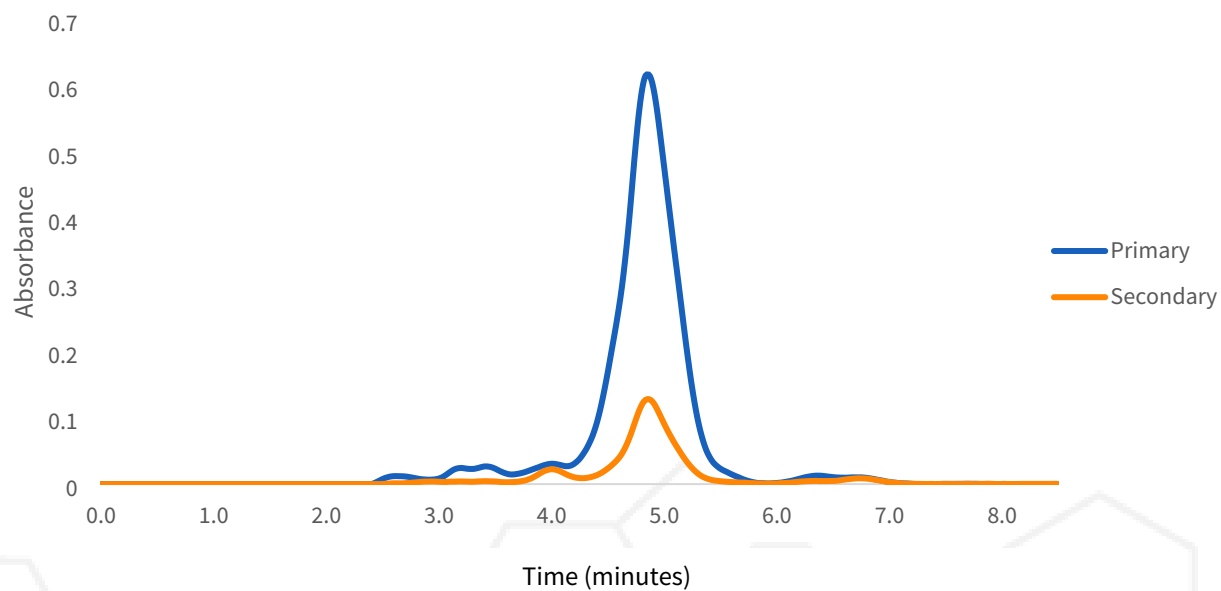

Sample Images



Change History


Date	User	Action
2025-07-18 12:27:21 -04:00		Test Recorded
2025-07-18 12:52:55 -04:00		Generated a CoA (revision 0)
2025-07-21 08:56:20 -04:00	DA	Added an image
2025-07-21 08:59:40 -04:00	DA	Changed Operator from "" to "DAIANA". Changed EdblProduct from "" to "D8 -D9- HHC - THC-P Strawberry Infused Gummies - 1500mg ". Changed Batch from "" to "MU0075".
2025-07-21 08:59:48 -04:00		Generated a CoA (revision 1)



Approved

07/18/2025

Date



Scan for Authenticity

The signatory confirms that the Operator has performed the sample preparation according to the LightLab User's Guide. This report is for quality assurance purposes only. These results relate only to the sample included on this report. Orange Photonics makes no claims as to the efficacy, safety, or risks associated with any detected or non-detected level of any compounds reported herein. Orange Photonics makes no claims regarding the adherence to sample preparation guidelines, by the operator, as outlined in the LightLab User's Guide.